

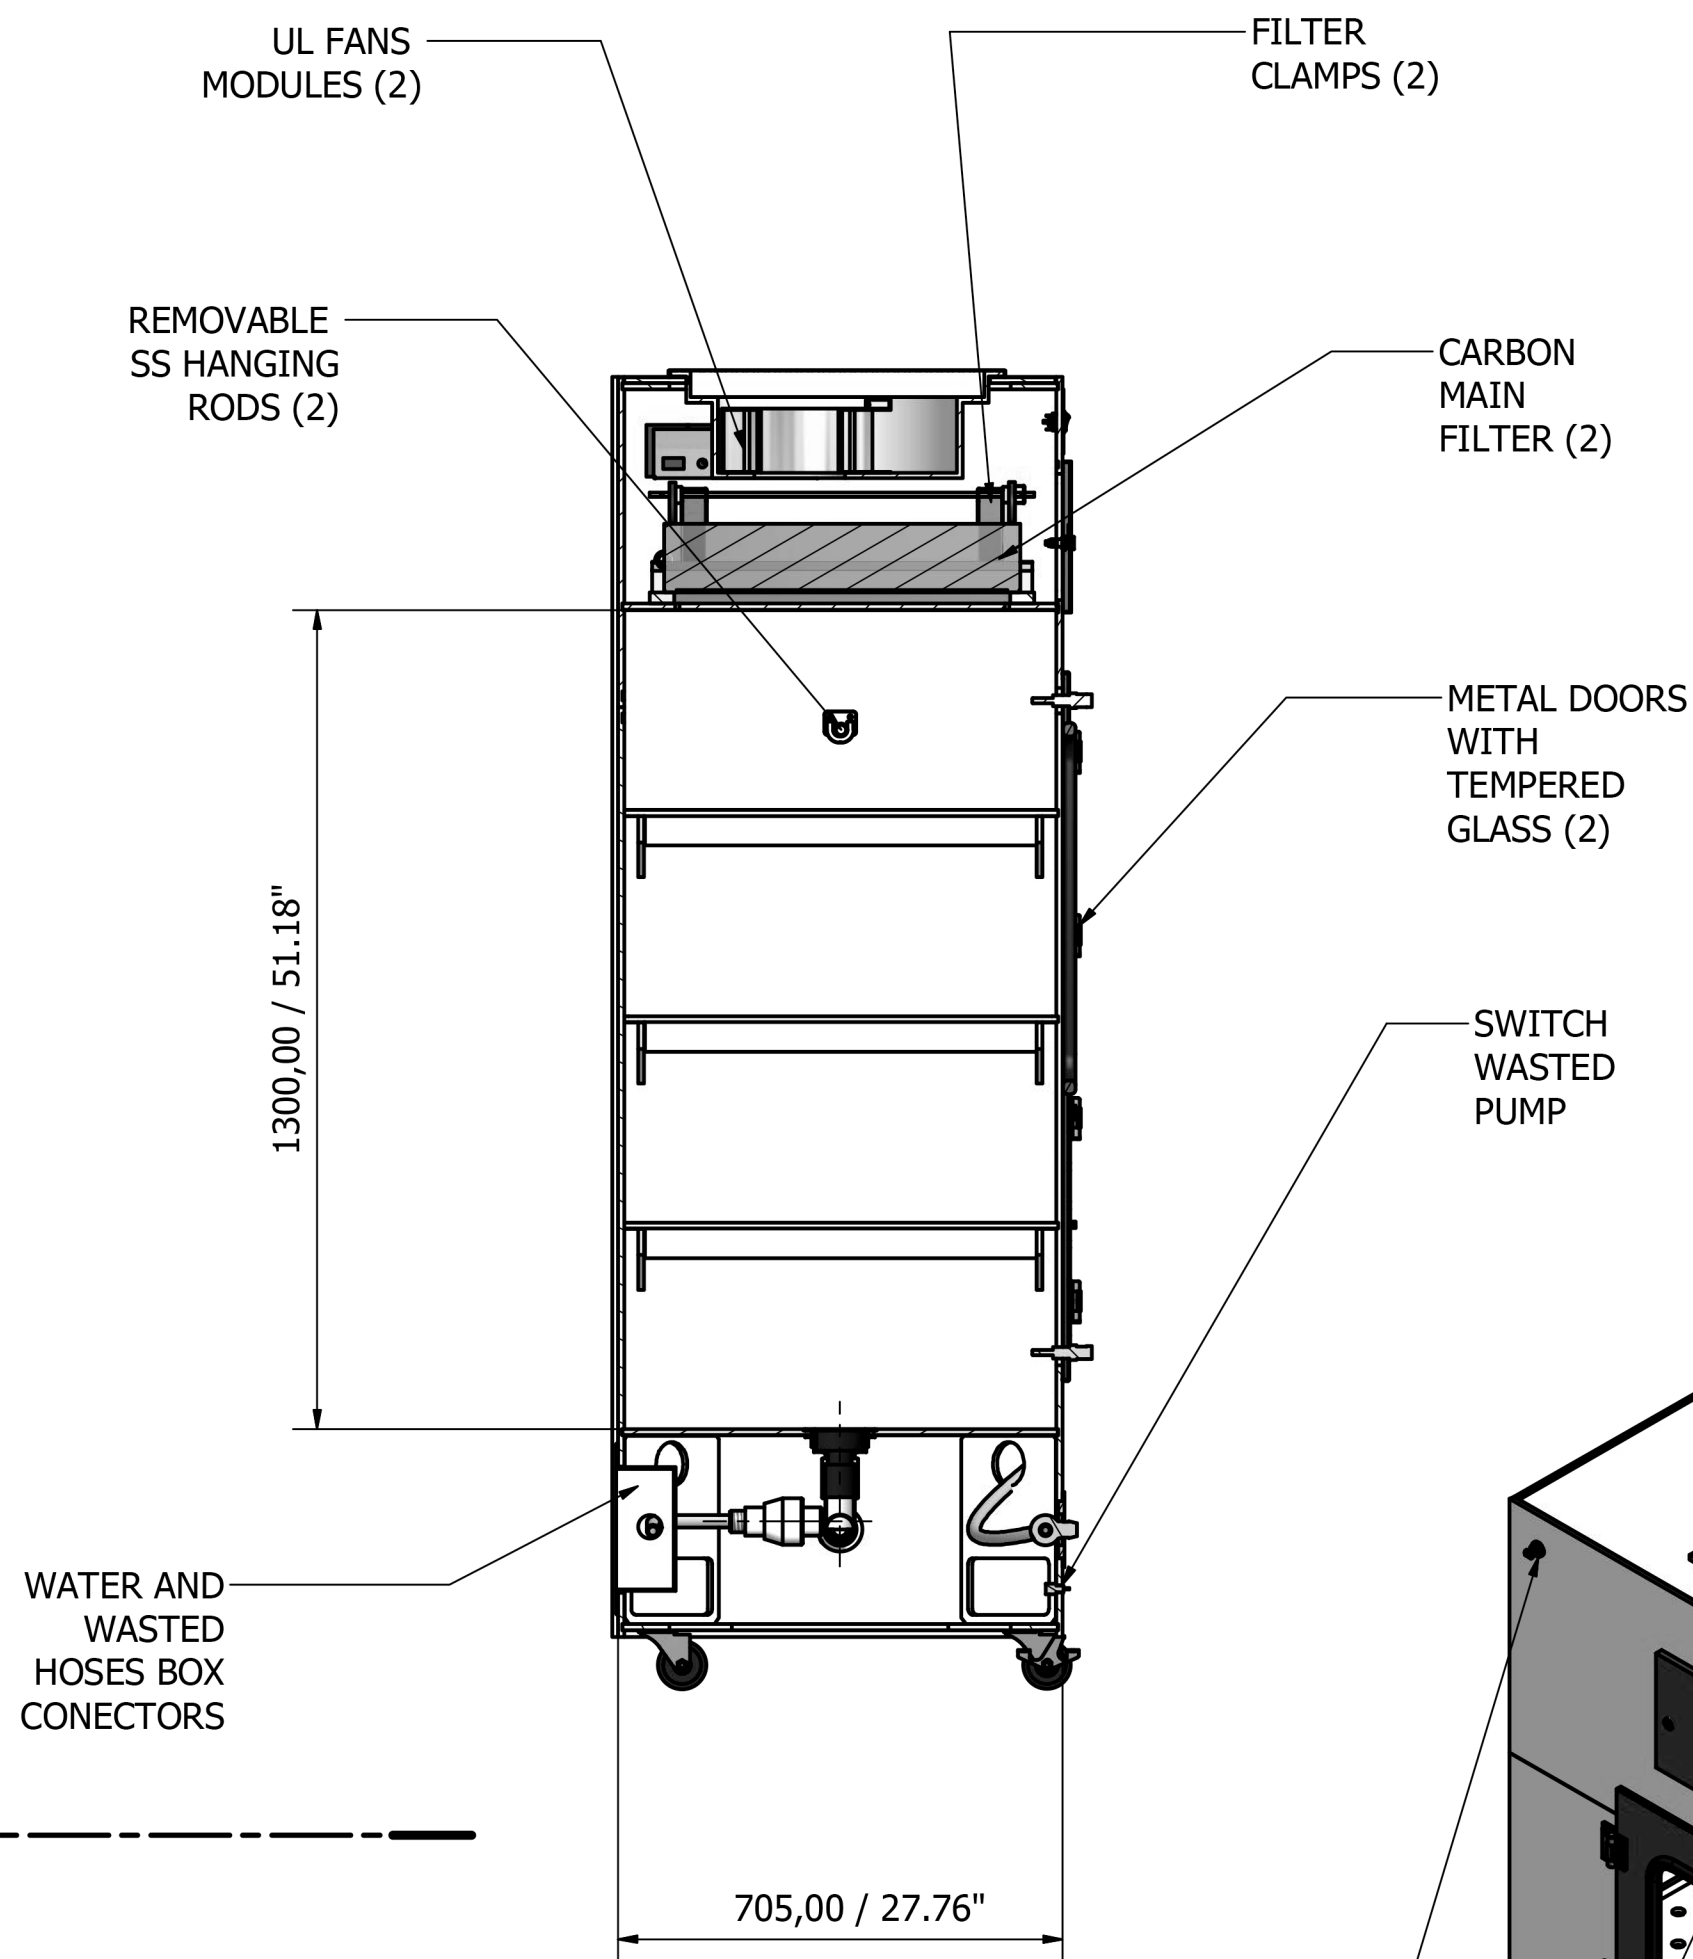
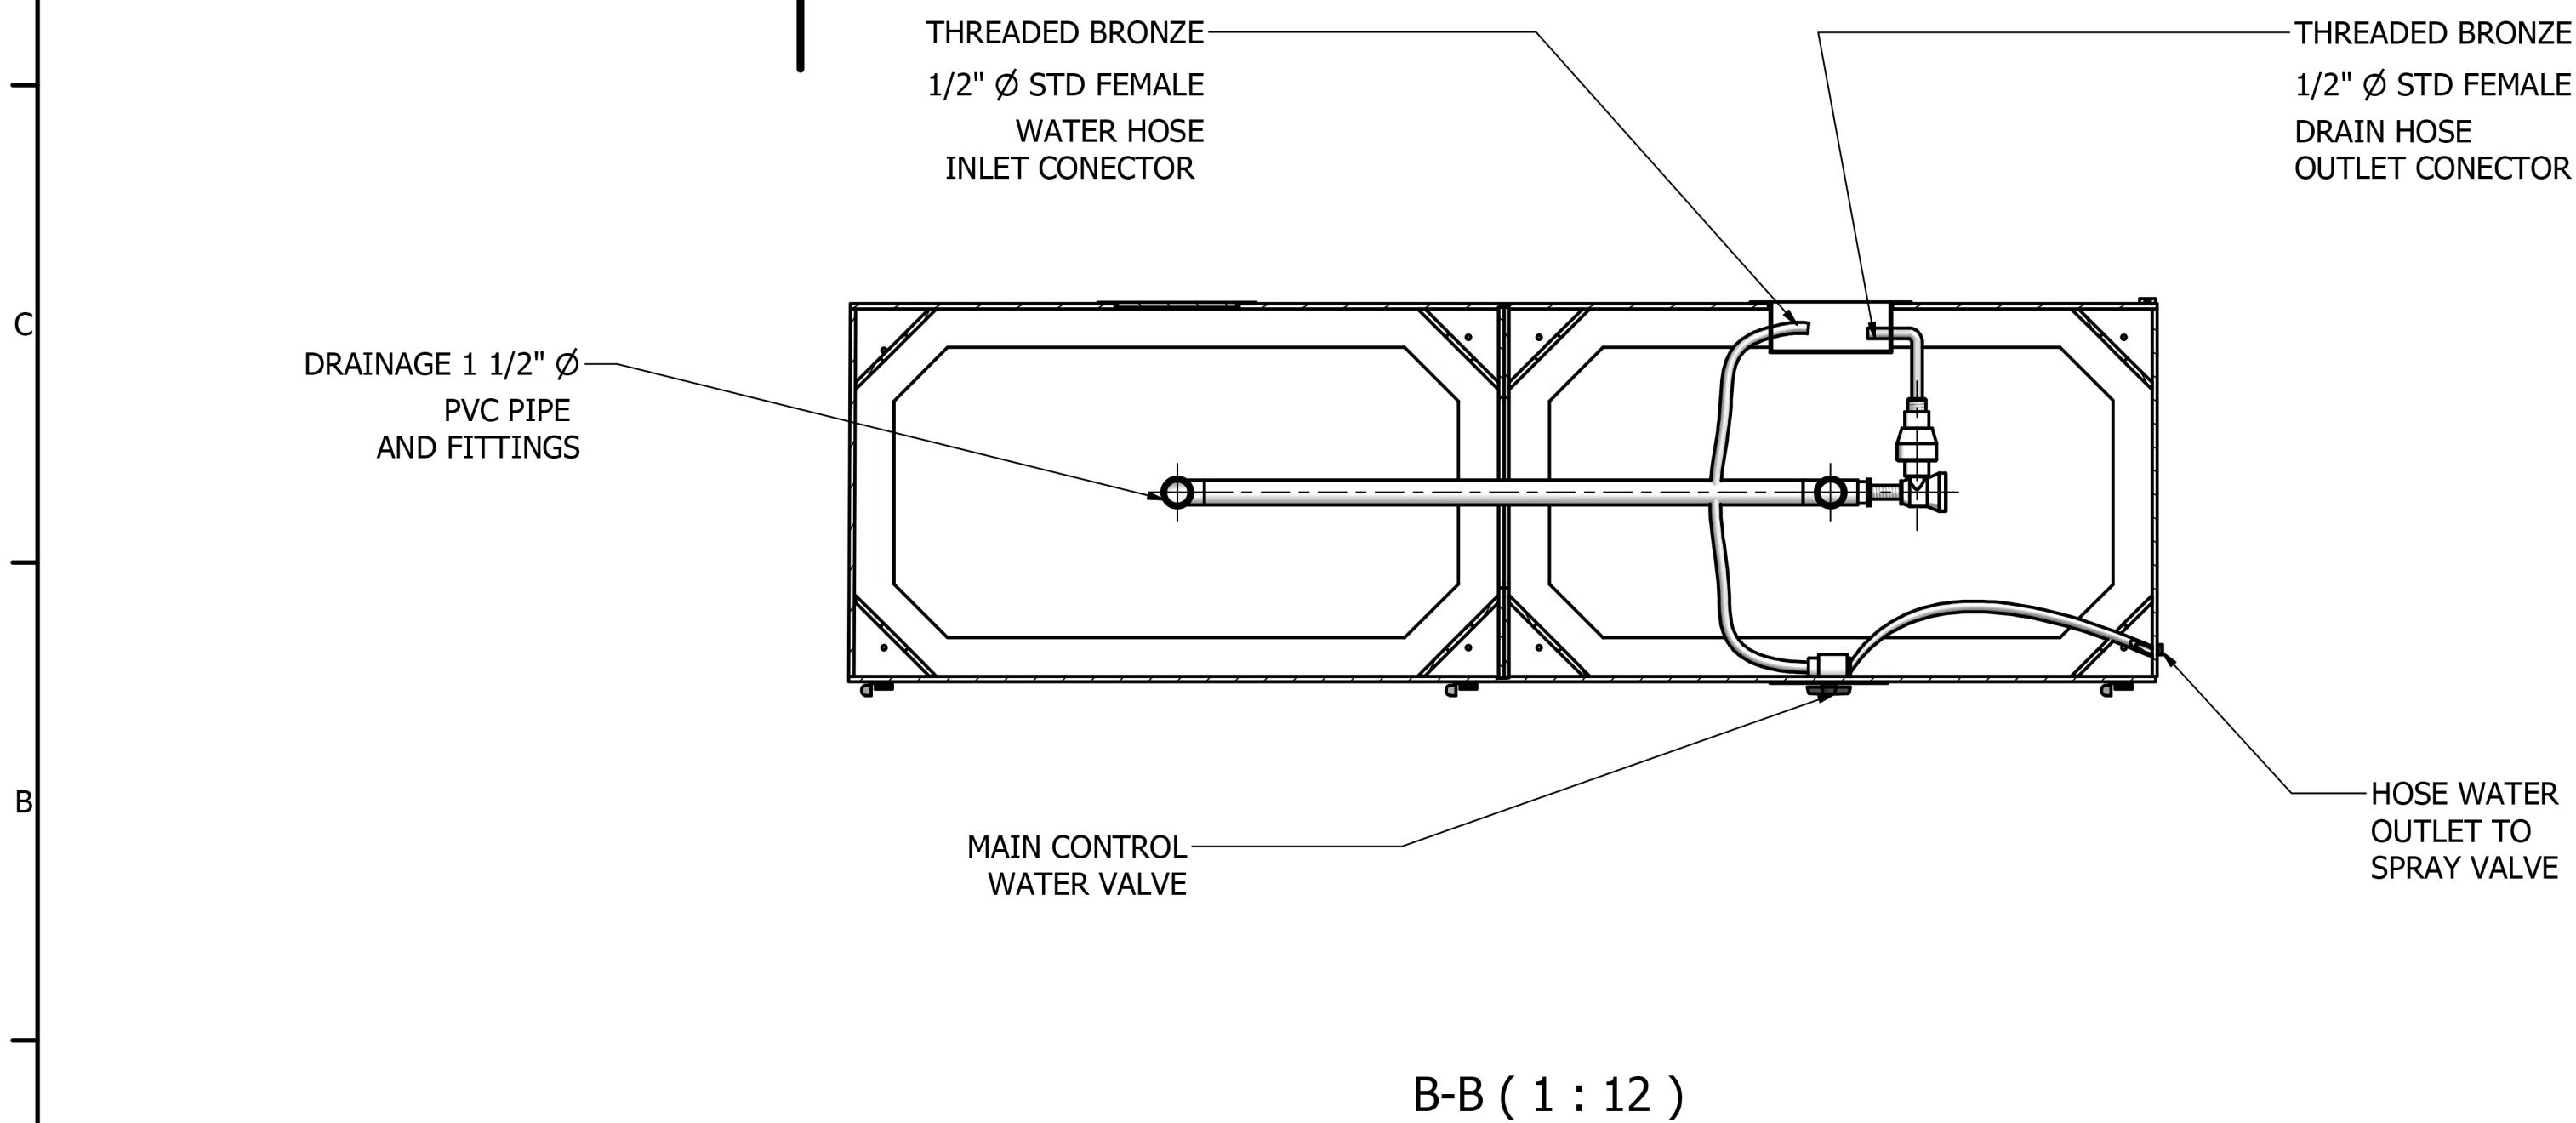


REVISION HISTORY				
ZONE	REV	DESCRIPTION	DATE	APPROVED
FAN LEVEL	1	UL FAN MODULE	7/06/2010	P CH
MAIN FILTER LEVEL	2	METAL CLAMPS	8/12/2011	P CH
RIGHT SIDE	3	METAL SHOEBOX	3/28/2012	P CH

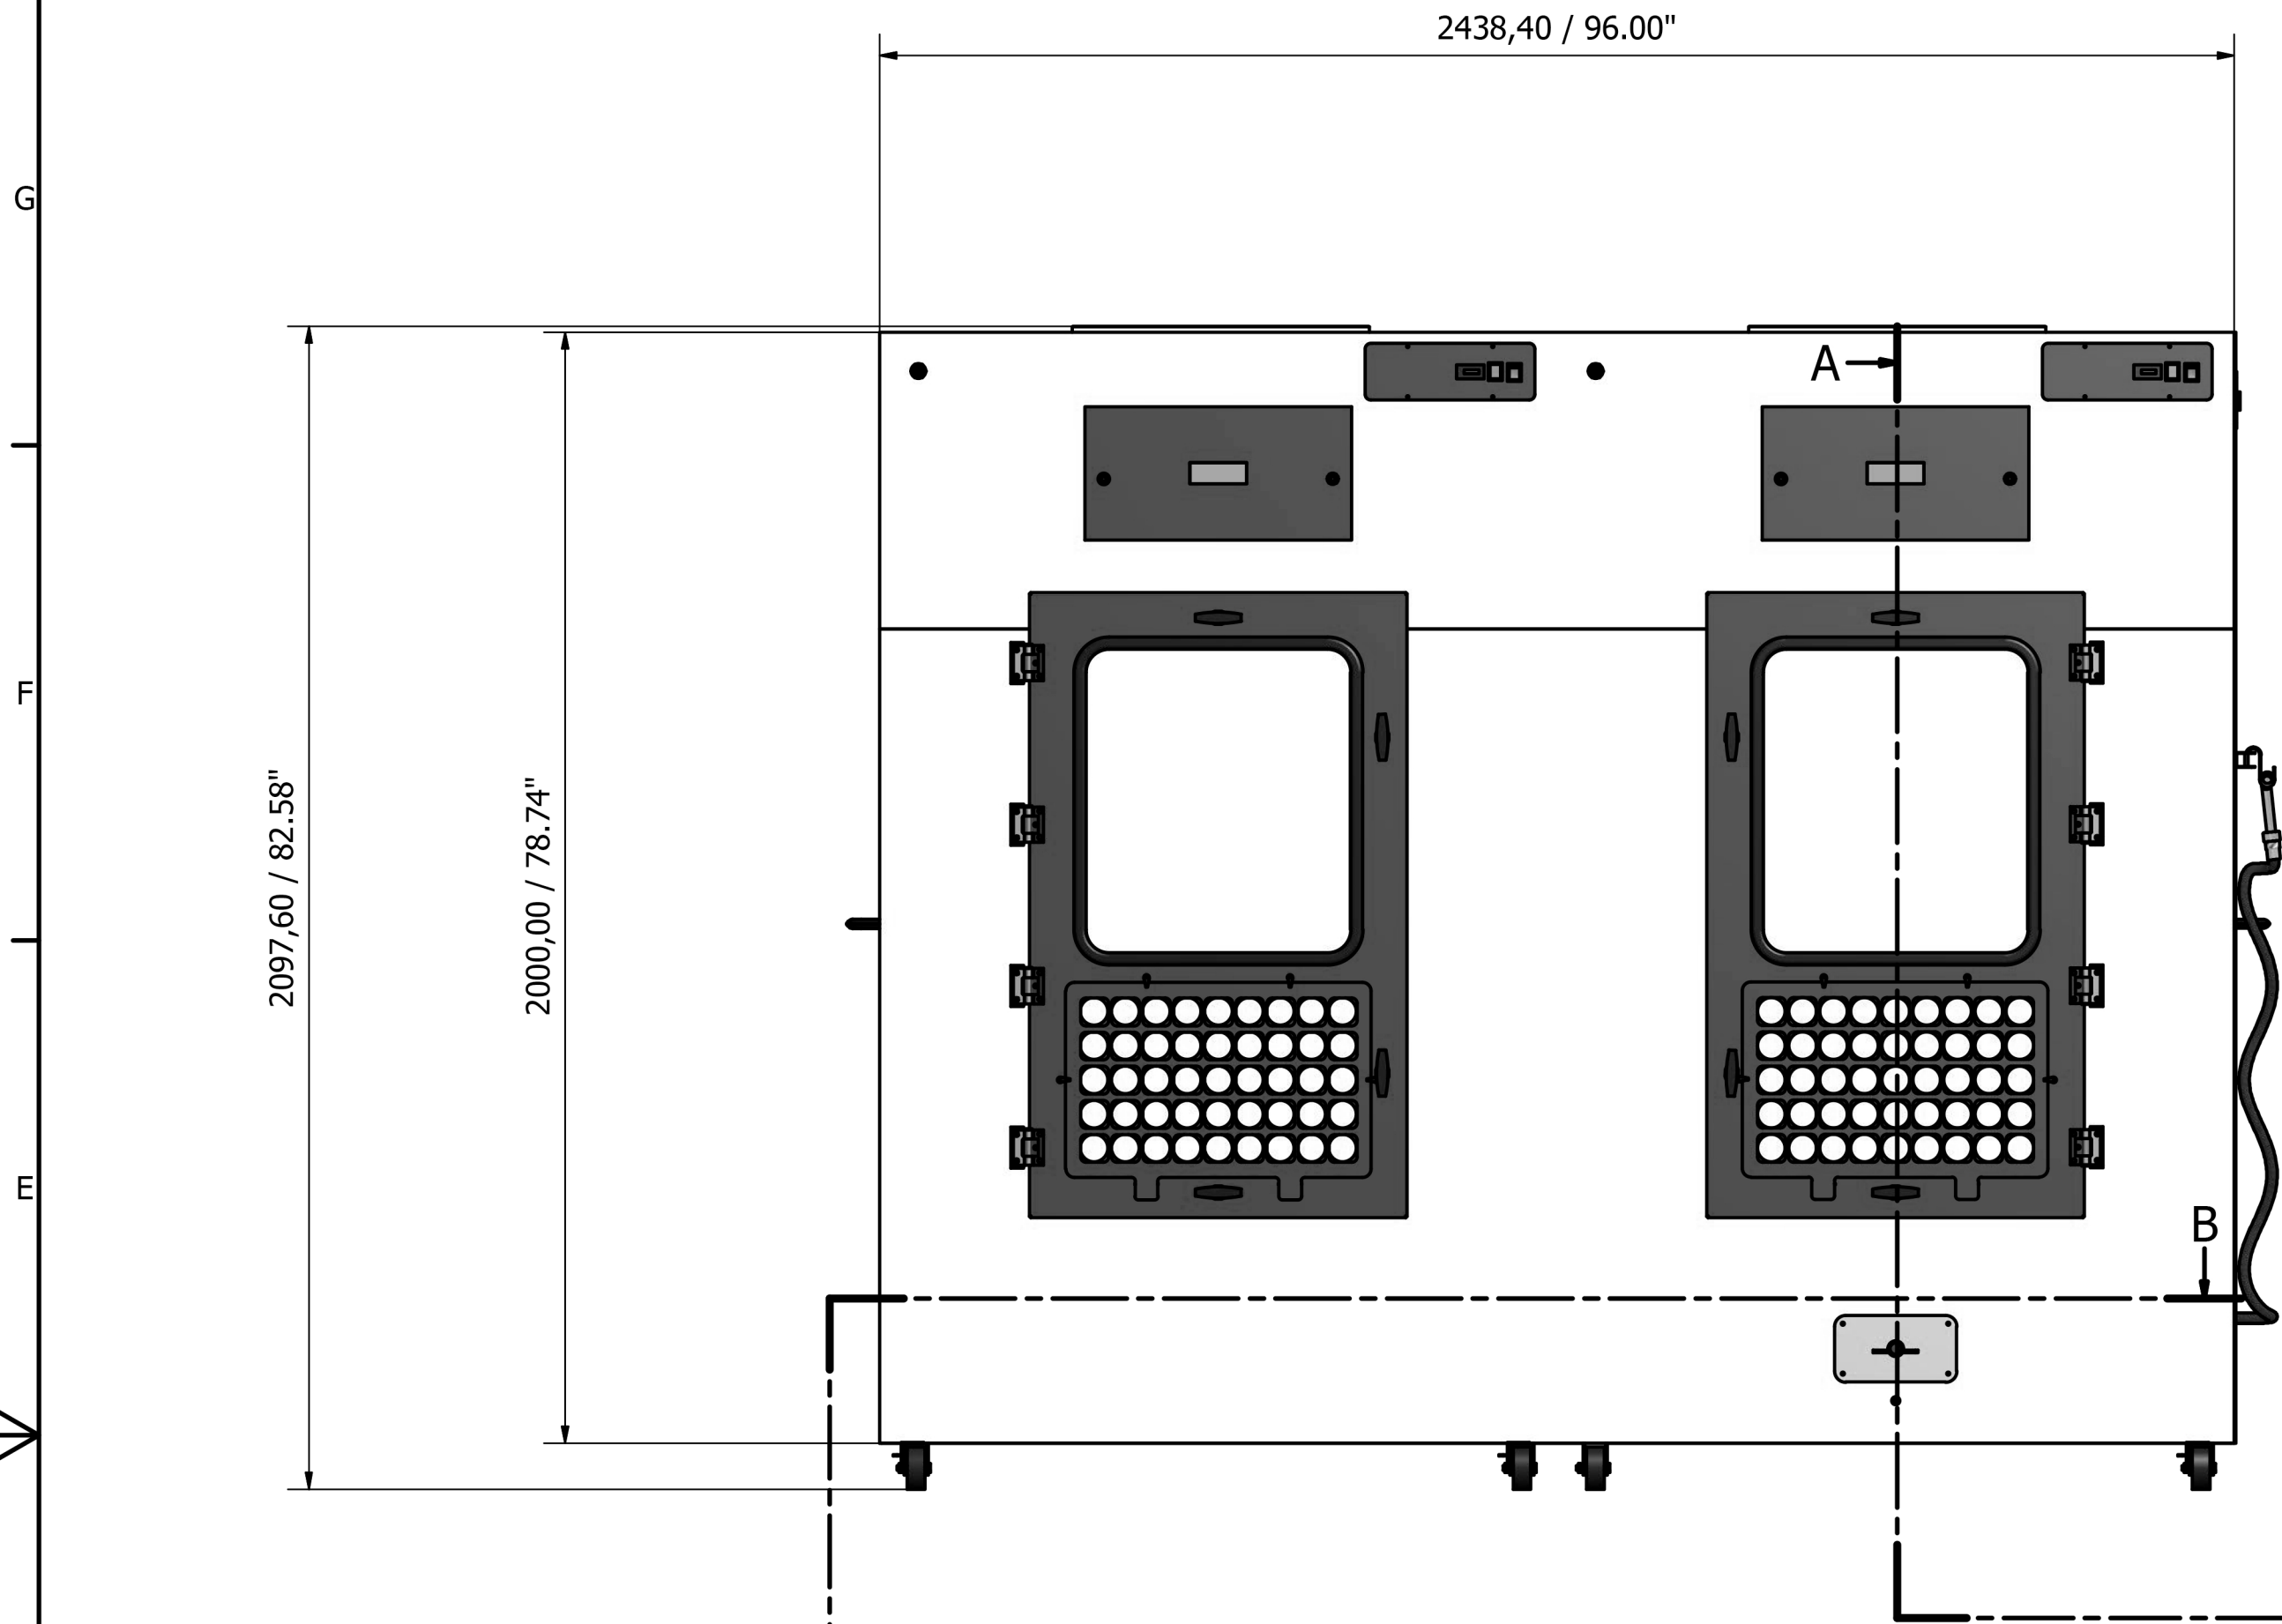

A-A (1 : 12)

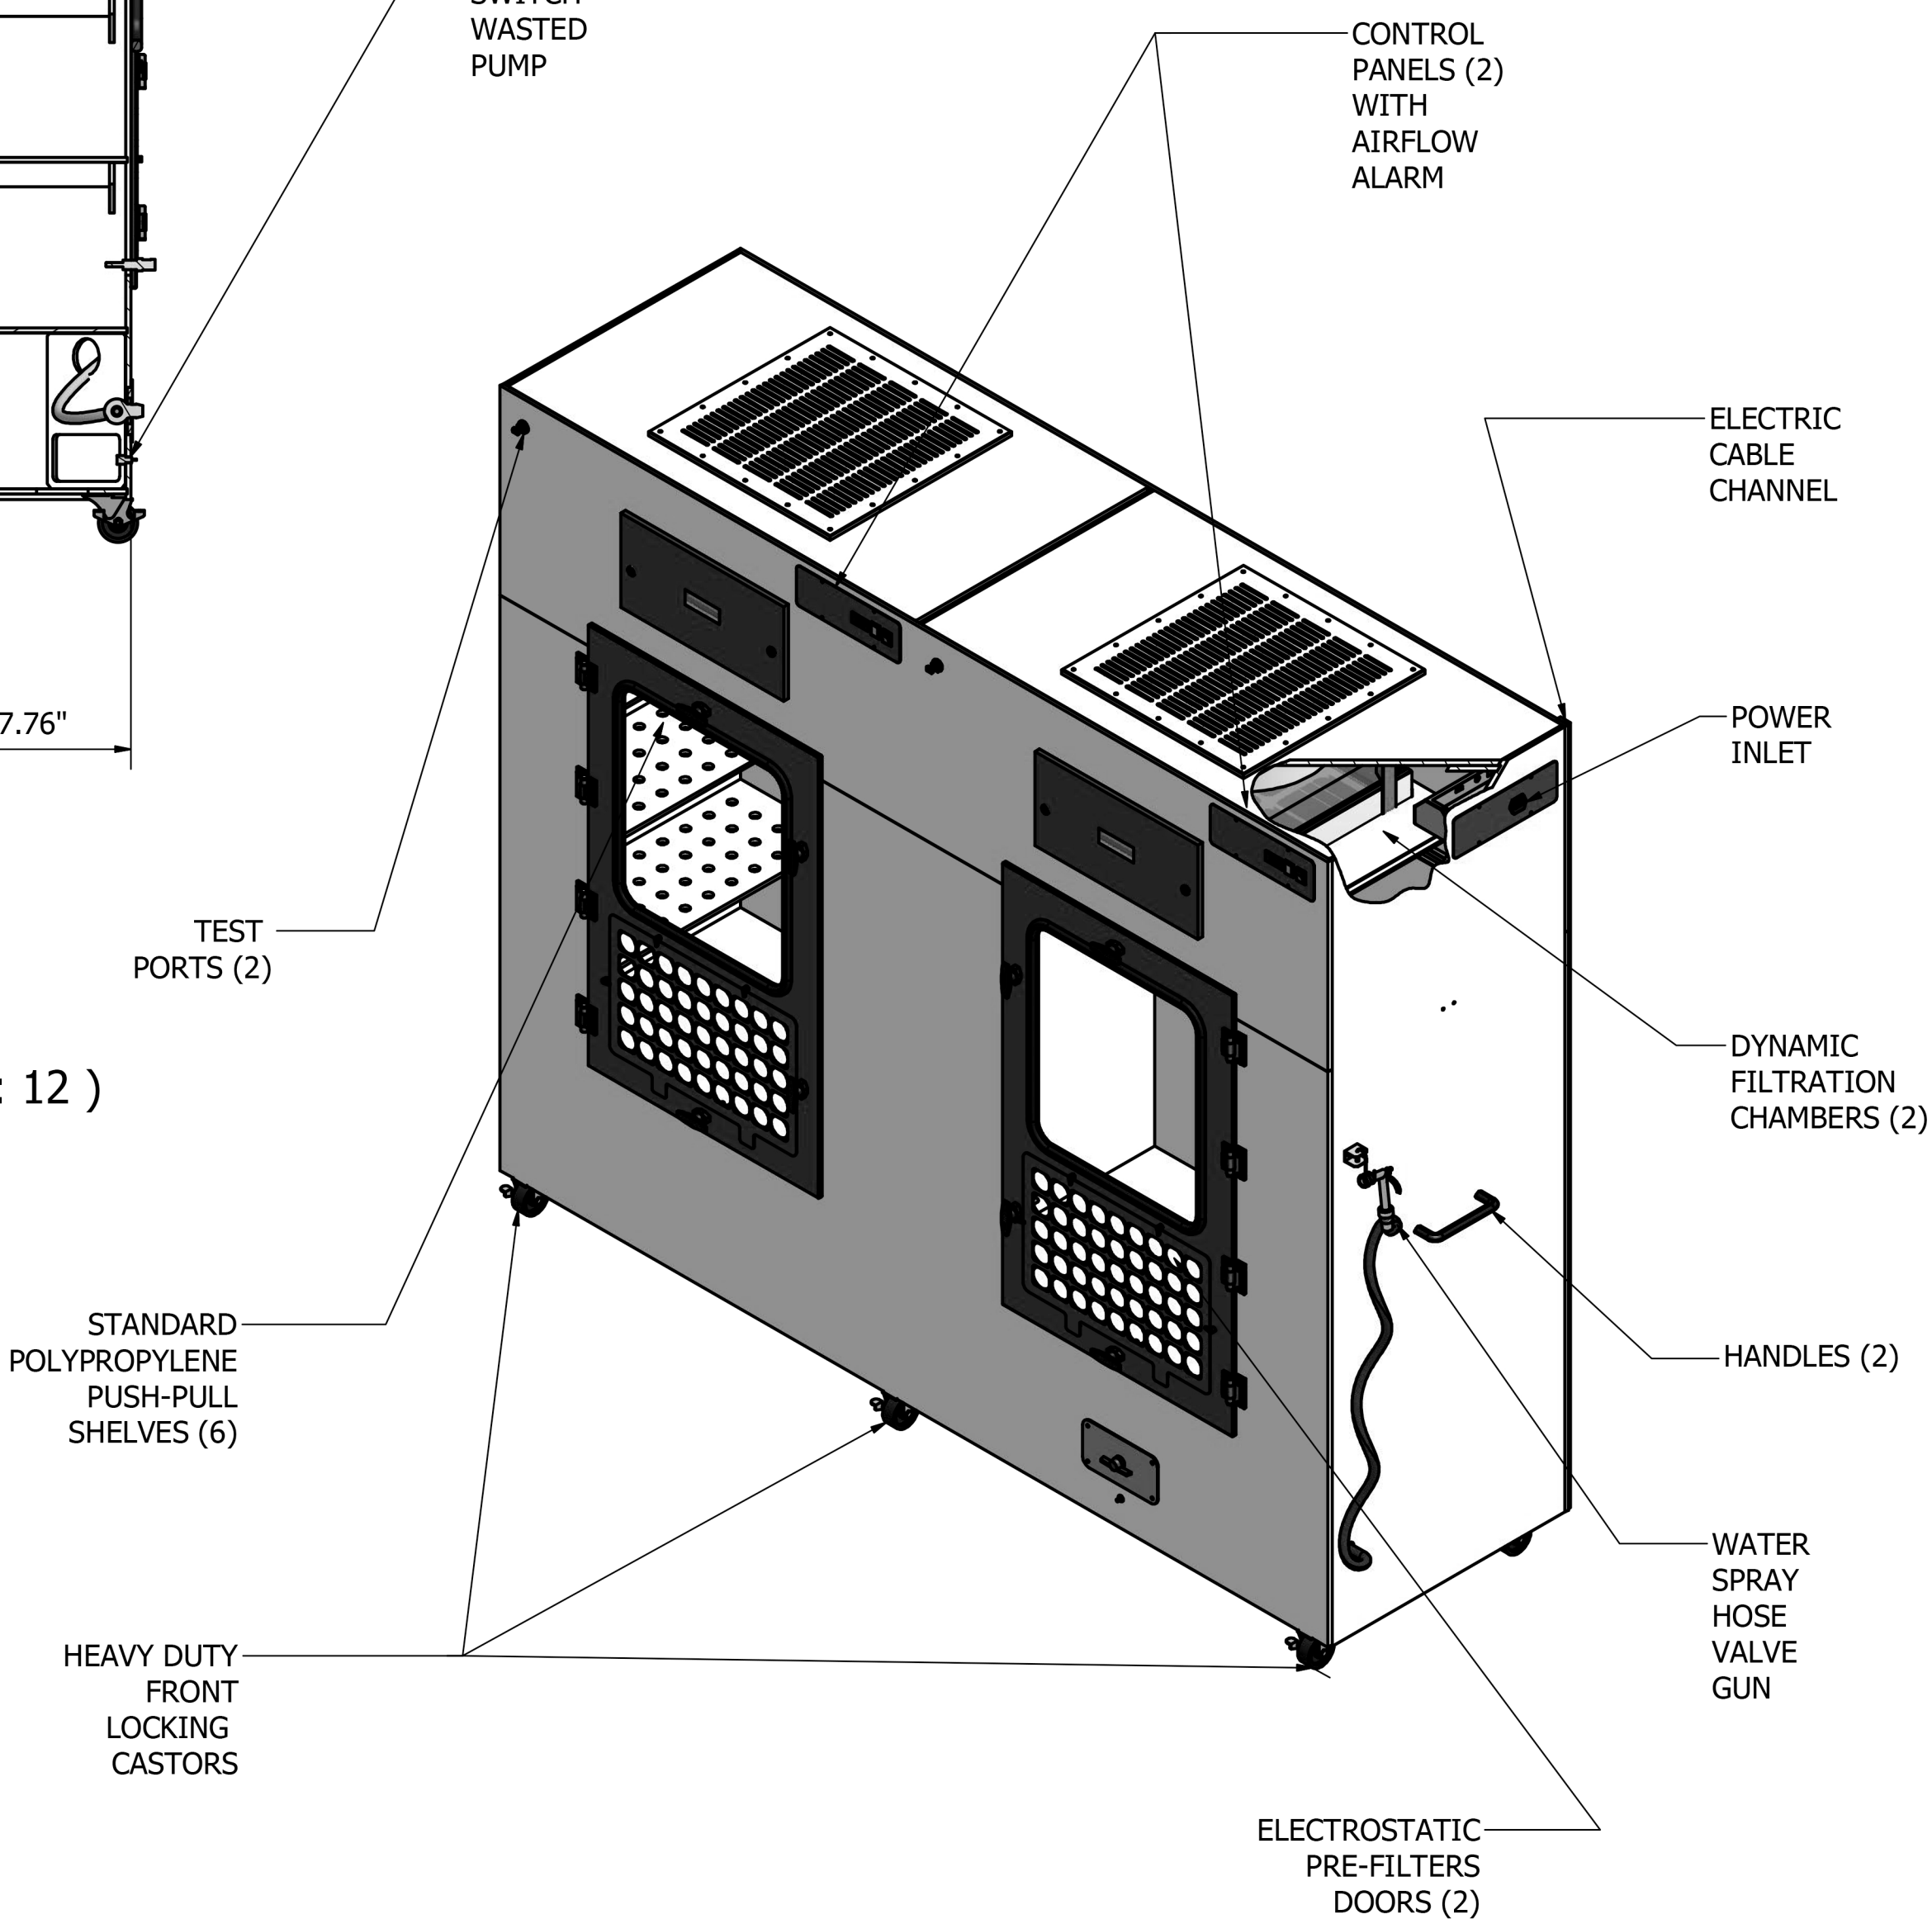

- NOTES:
1.0 CUSTOMER:

2.0 SUBMIT DRAWINGS FOR APPROVAL.
3.0 INCLUDED:
3.1 STANDARD ITEMS APPLIED.
3.2 PLUMBING PACKAGE.
3.3 SPRAY VALVE AND 1/2" X 6' HOSES FOR DRAINAGE AND COLD WATER WITH BRONZE FEMALE CONECTORS.
4.0 CABINET BUILT WITH 3/8" WHITE POLYPROPYLENE, SEAMLESS, NON-POROUS WATERTIGHT INSIDE, THERMALLY FUSE.
5.0 STANDARD MOLDED PLUG NEMA 4-14P
6.0 ELECTRICAL REQUIREMENTS 110V 6A 60 HZ

Designed by CFG	Checked by	Approved by	Date 8/25/2015	
			DC D96XT.2000UL SAFEKEEPER	
			DCD96XT-Gassem	Sheet 1 / 1